
## Sandeep Kumar Vashist

List of Publications by Year in descending order

Source: https://exaly.com/author-pdf/5073138/publications.pdf Version: 2024-02-01

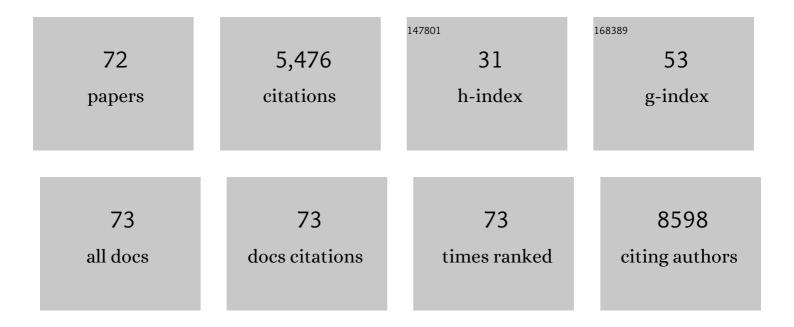

#	Article	IF	CITATIONS
1	Trends in Multiplex Immunoassays for In Vitro Diagnostics and Point-of-Care Testing. Diagnostics, 2021, 11, 1630.	2.6	5
2	Point-of-Care Technologies Enabling Next-Generation Healthcare Monitoring and Management. , 2019, ,		10
3	An Overview of Point-of-Care Technologies Enabling Next-Generation Healthcare Monitoring and Management. , 2019, , 1-25.		5
4	Smartphone-Based Point-of-Care Technologies for Mobile Healthcare. , 2019, , 27-79.		7
5	Commercially Available Smartphone-Based Personalized Mobile Healthcare Technologies. , 2019, , 81-115.		3
6	Point-of-Care Diabetes Management Softwares and Smart Applications. , 2019, , 117-132.		2
7	Paper-Based Point-of-Care Immunoassays. , 2019, , 133-155.		2
8	Lab-on-a-Chip-Based Point-of-Care Immunoassays. , 2019, , 157-175.		0
9	Multiplex Immunoassays. , 2019, , 177-196.		0
10	Bioanalytical Parameters in Immunoassays and Their Determination. , 2019, , 197-208.		0
11	Future Trends for the Next Generation of Personalized and Integrated Healthcare for Chronic Diseases. , 2019, , 209-223.		Ο
12	Wearable Technologies for Personalized Mobile Healthcare Monitoring and Management. , 2018, , 235-259.		6
13	Immunosensing procedures for carcinoembryonic antigen using graphene and nanocomposites. Biosensors and Bioelectronics, 2017, 89, 293-304.	10.1	31
14	Emerging Human Fetuin A Assays for Biomedical Diagnostics. Trends in Biotechnology, 2017, 35, 407-421.	9.3	15
15	A Smartphone-Based Colorimetric Reader for Human C-Reactive Protein Immunoassay. Methods in Molecular Biology, 2017, 1571, 343-356.	0.9	8
16	A rapid and highly sensitive immunoassay format for human lipocalin-2 using multiwalled carbon nanotubes. Biosensors and Bioelectronics, 2017, 93, 198-204.	10.1	6
17	Point-of-Care Diagnostics: Recent Advances and Trends. Biosensors, 2017, 7, 62.	4.7	154
18	Trends in in vitro diagnostics and mobile healthcare. Biotechnology Advances, 2016, 34, 137-138.	11.7	32

2

SANDEEP KUMAR VASHIST

#	Article	IF	CITATIONS
19	Microfluidic solutions enabling continuous processing and monitoring of biological samples: A review. Analytica Chimica Acta, 2016, 929, 1-22.	5.4	61
20	Surface plasmon resonance-based immunoassay for procalcitonin. Analytica Chimica Acta, 2016, 938, 129-136.	5.4	32
21	Bioanalytical advances in assays for C-reactive protein. Biotechnology Advances, 2016, 34, 272-290.	11.7	113
22	Chapter 5 Glycated haemoglobin (HbA1c) monitoring for diabetes diagnosis, management and therapy. , 2016, , 97-124.		1
23	Chapter 6 Diabetes management software and smart applications. , 2016, , 125-144.		1
24	Chapter 2 Blood glucose monitoring devices. , 2016, , 19-48.		0
25	Chapter 3 Non-invasive analytics for point-of-care testing of glucose. , 2016, , 49-74.		0
26	Chapter 1 Diabetes: a growing epidemic and the need for point-of-care testing. , 2016, , 1-18.		0
27	Chapter 4 Continuous glucose monitoring systems. , 2016, , 75-96.		0
28	Rapid sandwich ELISA-based in vitro diagnostic procedure for the highly-sensitive detection of human fetuin A. Biosensors and Bioelectronics, 2015, 67, 73-78.	10.1	35
29	A rapid sandwich immunoassay for human fetuin A using agarose-3-aminopropyltriethoxysilane modified microtiter plate. Analytica Chimica Acta, 2015, 883, 74-80.	5.4	9
30	Surface plasmon resonance-based immunoassay for human C-reactive protein. Analyst, The, 2015, 140, 4445-4452.	3.5	45
31	Recent advances in electrochemical biosensing schemes using graphene and graphene-based nanocomposites. Carbon, 2015, 84, 519-550.	10.3	202
32	Emerging Technologies for Next-Generation Point-of-Care Testing. Trends in Biotechnology, 2015, 33, 692-705.	9.3	583
33	Graphene-based rapid and highly-sensitive immunoassay for C-reactive protein using a smartphone-based colorimetric reader. Biosensors and Bioelectronics, 2015, 66, 169-176.	10.1	75
34	A smartphone-based colorimetric reader for bioanalytical applications using the screen-based bottom illumination provided by gadgets. Biosensors and Bioelectronics, 2015, 67, 248-255.	10.1	201
35	Commercial Smartphone-Based Devices and Smart Applications for Personalized Healthcare Monitoring and Management. Diagnostics, 2014, 4, 104-128.	2.6	196
36	Graphene-based immunoassay for human lipocalin-2. Analytical Biochemistry, 2014, 446, 96-101.	2.4	23

#	Article	IF	CITATIONS
37	Cellphone-based devices for bioanalytical sciences. Analytical and Bioanalytical Chemistry, 2014, 406, 3263-3277.	3.7	268
38	Immobilization of Antibodies and Enzymes on 3-Aminopropyltriethoxysilane-Functionalized Bioanalytical Platforms for Biosensors and Diagnostics. Chemical Reviews, 2014, 114, 11083-11130.	47.7	263
39	Surface plasmon resonance-based immunoassay for human fetuin A. Analyst, The, 2014, 139, 2237.	3.5	28
40	One-step kinetics-based immunoassay for the highly sensitive detection of C-reactive protein in less than 30min. Analytical Biochemistry, 2014, 456, 32-37.	2.4	62
41	One-step antibody immobilization-based rapid and highly-sensitive sandwich ELISA procedure for potential in vitro diagnostics. Scientific Reports, 2014, 4, 4407.	3.3	106
42	Bioluminescence assay for the highly sensitive detection of botulinum neurotoxin A activity. Analyst, The, 2013, 138, 6154.	3.5	16
43	Rapid and highly sensitive luciferase reporter assay for the automated detection of botulinum toxin in the centrifugal microfluidic LabDisk platform. RSC Advances, 2013, 3, 22046.	3.6	14
44	Graphene versus Multi-Walled Carbon Nanotubes for Electrochemical Glucose Biosensing. Materials, 2013, 6, 1011-1027.	2.9	69
45	A sub-picogram sensitive rapid chemiluminescent immunoassay for the detection of human fetuin A. Biosensors and Bioelectronics, 2013, 40, 297-302.	10.1	32
46	Continuous Glucose Monitoring Systems: A Review. Diagnostics, 2013, 3, 385-412.	2.6	194
47	Effect of 3-Aminopropyltriethoxysilane on the Electrocatalysis of Carbon Nanotubes for Reagentless Glucose Biosensing. Journal of Nanopharmaceutics and Drug Delivery, 2013, 1, 64-73.	0.3	3
48	Advances in Graphene-Based Sensors and Devices. Journal of Nanomedicine & Nanotechnology, 2012, 04,	1.1	8
49	Comparison of 1-Ethyl-3-(3-Dimethylaminopropyl) Carbodiimide Based Strategies to Crosslink Antibodies on Amine-Functionalized Platforms for Immunodiagnostic Applications. Diagnostics, 2012, 2, 23-33.	2.6	140
50	Rapid and simple preparation of a reagentless glucose electrochemical biosensor. Analyst, The, 2012, 137, 3800.	3.5	29
51	Mediatorless amperometric glucose biosensing using 3-aminopropyltriethoxysilane-functionalized graphene. Talanta, 2012, 99, 22-28.	5.5	46
52	Nanotechnology-Based Biosensors and Diagnostics: Technology Push versus Industrial/Healthcare Requirements. BioNanoScience, 2012, 2, 115-126.	3.5	64
53	Non-invasive glucose monitoring technology in diabetes management: A review. Analytica Chimica Acta, 2012, 750, 16-27.	5.4	467
54	Development of a Rapid Sandwich Enzyme Linked Immunoassay Procedure for the Highly Sensitive Detection of Human Lipocalin-2/NGAL. Procedia Chemistry, 2012, 6, 141-148.	0.7	9

#	Article	IF	CITATIONS
55	Comparative Study of the Developed Chemiluminescent, ELISA and SPR Immunoassay Formats for the Highly Sensitive Detection of Human Albumin. Procedia Chemistry, 2012, 6, 184-193.	0.7	14
56	Effect of antibody modifications on its biomolecular binding as determined by surface plasmon resonance. Analytical Biochemistry, 2012, 421, 336-338.	2.4	15
57	A method for regenerating gold surface for prolonged reuse of gold-coated surface plasmon resonance chip. Analytical Biochemistry, 2012, 423, 23-25.	2.4	10
58	Carbon nanotube bottles for incorporation, release and enhanced cytotoxic effect of cisplatin. Carbon, 2012, 50, 1625-1634.	10.3	86
59	Evaluation of apparent non-specific protein loss due to adsorption on sample tube surfaces and/or altered immunogenicity. Analyst, The, 2011, 136, 1406.	3.5	47
60	Effect of antibody immobilization strategies on the analytical performance of a surface plasmon resonance-based immunoassay. Analyst, The, 2011, 136, 4431.	3.5	140
61	Technology behind commercial devices for blood glucose monitoring in diabetes management: A review. Analytica Chimica Acta, 2011, 703, 124-136.	5.4	181
62	Interference of N-hydroxysuccinimide with bicinchoninic acid protein assay. Biochemical and Biophysical Research Communications, 2011, 411, 455-457.	2.1	13
63	Recent Advances in Quartz Crystal Microbalance-Based Sensors. Journal of Sensors, 2011, 2011, 1-13.	1.1	176
64	Multisubstrate-compatible ELISA procedures for rapid and high-sensitivity immunoassays. Nature Protocols, 2011, 6, 439-445.	12.0	144
65	Advances in carbon nanotube based electrochemical sensors for bioanalytical applications. Biotechnology Advances, 2011, 29, 169-188.	11.7	401
66	Sulfo-N-hydroxysuccinimide interferes with bicinchoninic acid protein assay. Analytical Biochemistry, 2011, 417, 156-158.	2.4	14
67	Delivery of drugs and biomolecules using carbon nanotubes. Carbon, 2011, 49, 4077-4097.	10.3	241
68	Microcantilevers for Sensing Applications. Measurement and Control, 2010, 43, 84-88.	1.8	25
69	Interfacing Carbon Nanotubes with Living Mammalian Cells and Cytotoxicity Issues. Chemical Research in Toxicology, 2010, 23, 1131-1147.	3.3	150
70	Development of a High Sensitivity Rapid Sandwich ELISA Procedure and Its Comparison with the Conventional Approach. Analytical Chemistry, 2010, 82, 7049-7052.	6.5	138
71	Specific immobilization of human immunoglobulin G on gold-coated silicon microcantilever array. , 2007, , .		0
72	In Vitro Diagnostics for COVID-19: State-of-the-Art, Future Directions and Role in Pandemic Response. ,		0

<sup>2</sup> 0, , .