
## Ching-Chou Wu

List of Publications by Year in descending order

Source: https://exaly.com/author-pdf/6550826/publications.pdf Version: 2024-02-01

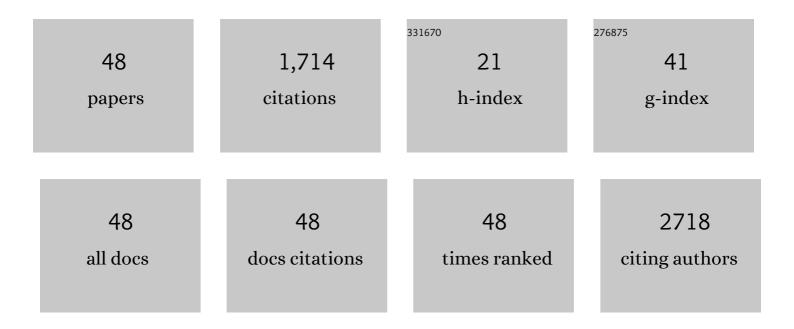

#	Article	IF	CITATIONS
1	A Label-Free Electrochemical Impedimetric Immunosensor with Biotinylated-Antibody for SARS-CoV-2 Nucleoprotein Detection in Saliva. Biosensors, 2022, 12, 265.	4.7	24
2	Dissolved Oxygen-Sensing Chip Integrating an Open Container Connected with a Position-Raised Channel for Estimation of Cellular Mitochondrial Activity. ACS Sensors, 2022, 7, 1808-1818.	7.8	2
3	A light-up "G-quadruplex nanostring―for label-free and selective detection of miRNA via duplex-specific nuclease mediated tandem rolling circle amplification. Nanomedicine: Nanotechnology, Biology, and Medicine, 2021, 32, 102339.	3.3	9
4	(Invited) The Microfluidic Chip Combining a Position-Raised Channel and Ultramicroelectrodes for Fast Estimation of Cellular Respiratory Activity. ECS Meeting Abstracts, 2021, MA2021-01, 1334-1334.	0.0	0
5	A Novel Biocompatible Herbal Extract-Loaded Hydrogel for Acne Treatment and Repair. Oxidative Medicine and Cellular Longevity, 2021, 2021, 1-13.	4.0	11
6	A Label-Free Impedimetric Genosensor for the Nucleic Acid Amplification-Free Detection of Extracted RNA of Dengue Virus. Sensors, 2020, 20, 3728.	3.8	14
7	Label-Free Impedimetric Immunosensors Modulated by Protein A/Bovine Serum Albumin Layer for Ultrasensitive Detection of Salbutamol. Sensors, 2020, 20, 771.	3.8	5
8	(Invited) Development of Cell-Based Microfluidic Chip for the Estimation of Cell Activity. ECS Meeting Abstracts, 2020, MA2020-01, 1993-1993.	0.0	0
9	Electrochemical sandwich immunoassay for quantification of therapeutic drugs based on the use of magnetic nanoparticles and silica nanoparticles. Journal of Electroanalytical Chemistry, 2019, 849, 113381.	3.8	6
10	Effect of Poly-I-Lysine Polycation on the Glucose Oxidase/Ferricyanide Composite-Based Second-Generation Blood Glucose Sensors. Sensors, 2019, 19, 1448.	3.8	12
11	A Microchip Electrophoresis Device Integrated with the Top–bottom Antiparallel Electrodes of Indium Tin Oxide to Detect Inorganic Ions by Contact Conductivity. Analytical Sciences, 2018, 34, 1231-1236.	1.6	2
12	A disposable non-enzymatic histamine sensor based on the nafion-coated copper phosphate electrodes for estimation of fish freshness. Electrochimica Acta, 2018, 283, 772-779.	5.2	25
13	An electrooxidative technique to fast fabricate copper phosphate electrodes capable of integrating high performance liquid chromatography for the label-free detection of fish freshness. Food Chemistry, 2018, 269, 16-23.	8.2	3
14	An impedimetric bioaffinity sensing chip integrated with the long-range DC-biased AC electrokinetic centripetal vortex produced in a high conductivity solution. Biomicrofluidics, 2018, 12, 044102.	2.4	4
15	Effect of the Chain Length of a Modified Layer and Surface Roughness of an Electrode on Impedimetric Immunosensors. Analytical Sciences, 2017, 33, 327-331.	1.6	6
16	Ionic Liquid-Modified Copper Phosphate Electrodes for the Detection of α-Amino Acids in a Weakly Alkaline Solution. Journal of the Electrochemical Society, 2016, 163, B768-B774.	2.9	3
17	A high sensitive impedimetric salbutamol immunosensor based on the gold nanostructure-deposited screen-printed carbon electrode. Journal of Electroanalytical Chemistry, 2016, 768, 27-33.	3.8	28
18	Development of a Capillary Electrophoresis Chip with Integrated Electrochemical Sensors. International Journal of Automation and Smart Technology, 2016, 6, 203-210.	0.4	0

Снілс-Снои Wu

#	Article	IF	CITATIONS
19	Enhanced Hydrophilicity and Biocompatibility of Dental Zirconia Ceramics by Oxygen Plasma Treatment. Materials, 2015, 8, 684-699.	2.9	66
20	An ultrasensitive label-free electrochemical impedimetric DNA biosensing chip integrated with a DC-biased AC electroosmotic vortex. Sensors and Actuators B: Chemical, 2015, 209, 61-68.	7.8	23
21	Fabrication of nanostructured copper phosphate electrodes for the detection of α-amino acids. Sensors and Actuators B: Chemical, 2015, 206, 584-591.	7.8	30
22	Geometric effect of copper nanoparticles electrodeposited on screen-printed carbon electrodes on the detection of $\hat{I}_{\pm}$ , $\hat{I}_{-}^2$ and $\hat{I}_{-}^3$ amino acids. Sensors and Actuators B: Chemical, 2013, 186, 270-277.	7.8	10
23	A label-free impedimetric DNA sensing chip integrated with AC electroosmotic stirring. Biosensors and Bioelectronics, 2013, 43, 348-354.	10.1	15
24	Electroosmotic Flow Control in Microfluidic Chips Using a Self-Assembled Monolayer as the Insulator of a Flow Field-Effect Transistor. Langmuir, 2012, 28, 11281-11285.	3.5	13
25	Title is missing!. Journal of Medical and Biological Engineering, 2012, 32, 163.	1.8	27
26	The simultaneous electrochemical detection of ascorbic acid, dopamine, and uric acid using graphene/size-selected Pt nanocomposites. Biosensors and Bioelectronics, 2011, 26, 3450-3455.	10.1	488
27	The open container-used microfluidic chip using IrOx ultramicroelectrodes for the in situ measurement of extracellular acidification. Biosensors and Bioelectronics, 2011, 26, 4191-4197.	10.1	16
28	Effect of polydimethylsiloxane surfaces silanized with different nitrogen-containing groups on the adhesion progress of epithelial cells. Surface and Coatings Technology, 2011, 205, 3182-3189.	4.8	22
29	Preparation and properties of gold nanoparticle-electrodeposited titanium substrates with Arg-Gly-Asp-Cys peptides. Journal of Materials Science: Materials in Medicine, 2010, 21, 1511-1519.	3.6	17
30	A Clark-type oxygen chip for in situ estimation of the respiratory activity of adhering cells. Talanta, 2010, 81, 228-234.	5.5	52
31	Development of an enrofloxacin immunosensor based on label-free electrochemical impedance spectroscopy. Talanta, 2009, 79, 62-67.	5.5	50
32	Study on the Cell Mechanics of MDCK Cells by Elastic Micro-pillars Arrays. , 2007, , .		1
33	Deregulation of AP-1 Proteins in Collagen Gel-induced Epithelial Cell Apoptosis Mediated by Low Substratum Rigidity. Journal of Biological Chemistry, 2007, 282, 752-763.	3.4	28
34	A new method for detection of endotoxin on polymyxin B-immobilized gold electrodes. Electrochemistry Communications, 2007, 9, 1206-1211.	4.7	61
35	Microfluidic chip integrated with amperometric detector array for in situ estimating oxygen consumption characteristics of single bovine embryos. Sensors and Actuators B: Chemical, 2007, 125, 680-687.	7.8	40
36	Oxygen consumption of cell suspension in a poly(dimethylsiloxane) (PDMS) microchannel estimated by scanning electrochemical microscopy. Analyst, The, 2006, 131, 1006.	3.5	33

Снімс-Снои Wu

#	Article	IF	CITATIONS
37	Oxygen Permeability of Surface-modified Poly(dimethylsiloxane) Characterized by Scanning Electrochemical Microscopy. Chemistry Letters, 2006, 35, 234-235.	1.3	103
38	Electrochemical evaluation of avidin–biotin interaction on self-assembled gold electrodes. Electrochimica Acta, 2005, 50, 3660-3666.	5.2	71
39	Measurement of diffusion and partition coefficients of ferrocyanide in protein-immobilized membranes. Analytica Chimica Acta, 2005, 532, 209-214.	5.4	18
40	Impedance spectral studies of self-assembly of alkanethiols with different chain lengths using different immobilization strategies on Au electrodes. Analytica Chimica Acta, 2005, 554, 43-51.	5.4	89
41	Fabrication of miniature Clark oxygen sensor integrated with microstructure. Sensors and Actuators B: Chemical, 2005, 110, 342-349.	7.8	96
42	Mechanical properties of collagen gels derived from rats of different ages. Journal of Biomaterials Science, Polymer Edition, 2005, 16, 1261-1275.	3.5	53
43	Estimating the thickness of hydrated ultrathin poly(o-phenylenediamine) film by atomic force microscopy. Analytica Chimica Acta, 2004, 505, 239-246.	5.4	20
44	Three-Electrode Electrochemical Detector and Platinum Film Decoupler Integrated with a Capillary Electrophoresis Microchip for Amperometric Detection. Analytical Chemistry, 2003, 75, 947-952.	6.5	87
45	Vagal innervation of the gastrointestinal tract arises from dorsal motor nucleus while that of the heart largely from nucleus ambiguus in the cat. Journal of the Autonomic Nervous System, 1998, 70, 38-50.	1.9	26
46	The depressor caudal ventrolateral medulla: Its correlation with the pressor dorsomedial and ventrolateral medulla and the depressor paramedian reticular nucleus. Journal of the Autonomic Nervous System, 1998, 70, 103-114.	1.9	5
47	On-column amperometric detection for capillary electrophoresis microchips with electric field decoupler. , 0, , .		Ο
48	A novel method of measuring the thickness of hydrated ultrathin polymer film by the force curve of atomic force microscopy. , 0, , .		0