
Christoph Lerche

List of Publications by Year in descending order

Source: https://exaly.com/author-pdf/8497345/publications.pdf Version: 2024-02-01

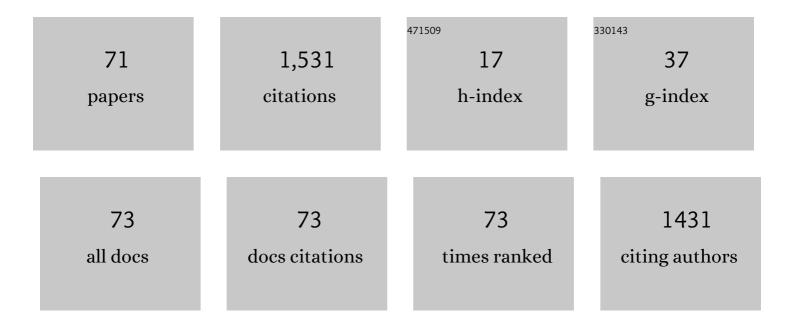

CHRISTORN | FRCHE

#	Article	IF	CITATIONS
1	Infrared exponent for gluon and ghost propagation in Landau gauge QCD. Physical Review D, 2002, 65, .	4.7	249
2	Depth of /spl gamma/-ray interaction within continuous crystals from the width of its scintillation light-distribution. IEEE Transactions on Nuclear Science, 2005, 52, 560-572.	2.0	117
3	MR compatibility aspects of a silicon photomultiplier-based PET/RF insert with integrated digitisation. Physics in Medicine and Biology, 2014, 59, 5119-5139.	3.0	105
4	A Digital Preclinical PET/MRI Insert and Initial Results. IEEE Transactions on Medical Imaging, 2015, 34, 2258-2270.	8.9	97
5	Predicting IDH genotype in gliomas using FET PET radiomics. Scientific Reports, 2018, 8, 13328.	3.3	90
6	Towards Software-Based Real-Time Singles and Coincidence Processing of Digital PET Detector Raw Data. IEEE Transactions on Nuclear Science, 2013, 60, 1550-1559.	2.0	73
7	Performance tests of two portable mini gamma cameras for medical applications. Medical Physics, 2006, 33, 4210-4220.	3.0	59
8	Initial PET performance evaluation of a preclinical insert for PET/MRI with digital SiPM technology. Physics in Medicine and Biology, 2016, 61, 2851-2878.	3.0	59
9	FET PET Radiomics for Differentiating Pseudoprogression from Early Tumor Progression in Glioma Patients Post-Chemoradiation. Cancers, 2020, 12, 3835.	3.7	55
10	Dependency of Energy-, Position- and Depth of Interaction Resolution on Scintillation Crystal Coating and Geometry. IEEE Transactions on Nuclear Science, 2008, 55, 1344-1351.	2.0	44
11	TRIMAGE: A dedicated trimodality (PET/MR/EEG) imaging tool for schizophrenia. European Psychiatry, 2018, 50, 7-20.	0.2	40
12	Advances in Clinical PET/MRI Instrumentation. PET Clinics, 2016, 11, 95-103.	3.0	38
13	Comparison of EEG microstates with resting state fMRI and FDGâ€PET measures in the default mode network via simultaneously recorded trimodal (PET/MR/EEC) data. Human Brain Mapping, 2021, 42, 4122-4133.	3.6	32
14	Data Processing for a High Resolution Preclinical PET Detector Based on Philips DPC Digital SiPMs. IEEE Transactions on Nuclear Science, 2015, 62, 669-678.	2.0	31
15	SiPM based preclinical PET/MR insert for a human 3T MR: first imaging experiments. , 2011, , .		30
16	PET Performance Evaluation of a Pre-Clinical SiPM-Based MR-Compatible PET Scanner. IEEE Transactions on Nuclear Science, 2015, 62, 784-790.	2.0	30
17	Design concept of world's first preclinical PET/MR insert with fully digital silicon photomultiplier technology. , 2012, , .		27
18	PESIC: An Integrated Front-End for PET Applications. IEEE Transactions on Nuclear Science, 2008, 55, 27-33.	2.0	26

CHRISTOPH LERCHE

#	Article	IF	CITATIONS
19	Multimodal Fingerprints of Resting State Networks as assessed by Simultaneous Trimodal MR-PET-EEG Imaging. Scientific Reports, 2017, 7, 6452.	3.3	23
20	Excitatory–inhibitory balance within EEG microstates and resting-state fMRI networks: assessed via simultaneous trimodal PET–MR–EEG imaging. Translational Psychiatry, 2021, 11, 60.	4.8	21
21	mGluR5 receptor availability is associated with lower levels of negative symptoms and better cognition in male patients with chronic schizophrenia. Human Brain Mapping, 2020, 41, 2762-2781.	3.6	20
22	AMIC: An Expandable Front-End for Gamma-Ray Detectors With Light Distribution Analysis Capabilities. IEEE Transactions on Nuclear Science, 2011, 58, 1641-1646.	2.0	16
23	Software-Based Real-Time Acquisition and Processing of PET Detector Raw Data. IEEE Transactions on Biomedical Engineering, 2016, 63, 316-327.	4.2	16
24	Scatter Correction Based on GPU-Accelerated Full Monte Carlo Simulation for Brain PET/MRI. IEEE Transactions on Medical Imaging, 2020, 39, 140-151.	8.9	15
25	DOI measurement with monolithic scintillation crystals: A primary performance evaluation. , 2007, , .		14
26	The Jülich Experience With Simultaneous 3T MR-BrainPET: Methods and Technology. IEEE Transactions on Radiation and Plasma Medical Sciences, 2019, 3, 352-362.	3.7	14
27	Simultaneous trimodal PET-MR-EEG imaging: Do EEG caps generate artefacts in PET images?. PLoS ONE, 2017, 12, e0184743.	2.5	11
28	PET attenuation correction for rigid MR Tx/Rx coils from ¹⁷⁶ Lu background activity. Physics in Medicine and Biology, 2018, 63, 035039.	3.0	11
29	Static FET PET radiomics for the differentiation of treatment-related changes from glioma progression. Journal of Neuro-Oncology, 2022, 159, 519-529.	2.9	11
30	PET/MR Synchronization by Detection of Switching Gradients. IEEE Transactions on Nuclear Science, 2015, 62, 650-657.	2.0	9
31	Simultaneous PET-MR-EEG: Technology, Challenges and Application in Clinical Neuroscience. IEEE Transactions on Radiation and Plasma Medical Sciences, 2019, 3, 377-385.	3.7	9
32	Maximum likelihood based positioning and energy correction for pixelated solid state PET detectors. , 2011, , .		8
33	Design and Characterization of a Gradient-Transparent RF Copper Shield for PET Detector Modules in Hybrid MR-PET Imaging. IEEE Transactions on Nuclear Science, 2017, 64, 1118-1127.	2.0	8
34	Application and performance of an ML-EM algorithm in NEXT. Journal of Instrumentation, 2017, 12, P08009-P08009.	1.2	8
35	Two Decades of Brain Tumour Imaging with O-(2-[18F]fluoroethyl)-L-tyrosine PET: The Forschungszentrum JÃ1⁄4lich Experience. Cancers, 2022, 14, 3336.	3.7	8
36	Improved Digital Pulse Height Estimation for PET Detectors Using LMS Adaptive Filters. IEEE Transactions on Nuclear Science, 2008, 55, 48-53.	2.0	7

#	ARTICLE	lF	CITATIONS
37	xmlns:mml="http://www.w3.org/1998/Math/MathML" altimg="si2.gif" overflow="scroll"> <mml:mi>LSO</mml:mi> <mml:mo>+</mml:mo> <mml:mi>PSPMT</mml:mi> PET system using low pass filter interpolation and digital constant fraction discriminator techniques. Nuclear Instruments and Methods in Physics Research, Section A: Accelerators,	1.6	7
38	Spectrometers, Detectors and Associated Equipment, 2009, 604, 347-350. Alternative headphones for patient noise protection and communication in PET-MR studies of the brain. EJNMMI Research, 2018, 8, 106.	2.5	7
39	A Novel J-Shape Antenna Array for Simultaneous MR-PET or MR-SPECT Imaging. IEEE Transactions on Medical Imaging, 2022, 41, 1104-1113.	8.9	7
40	mGluR5 binding changes during a mismatch negativity task in a multimodal protocol with [11C]ABP688 PET/MR-EEG. Translational Psychiatry, 2022, 12, 6.	4.8	7
41	Calibration and stability of a SiPM-based simultaneous PET/MR insert. Nuclear Instruments and Methods in Physics Research, Section A: Accelerators, Spectrometers, Detectors and Associated Equipment, 2013, 702, 50-53.	1.6	6
42	Maximum likelihood positioning and energy correction for scintillation detectors. Physics in Medicine and Biology, 2016, 61, 1650-1676.	3.0	6
43	Resolution modeling in projection space using a factorized multi-block detector response function for PET image reconstruction. Physics in Medicine and Biology, 2019, 64, 145012.	3.0	6
44	High-throughput, accurate Monte Carlo simulation on CPU hardware for PET applications. Physics in Medicine and Biology, 2021, 66, 185001.	3.0	5
45	Bias evaluation and reduction in 3D OP-OSEM reconstruction in dynamic equilibrium PET studies with 11C-labeled for binding potential analysis. PLoS ONE, 2021, 16, e0245580.	2.5	5
46	<scp>mGluR₅</scp> and <scp>GABA_A</scp> receptorâ€specific parametric <scp>PET</scp> atlas construction— <scp>PET</scp> / <scp>MR</scp> data processing pipeline, validation, and application. Human Brain Mapping, 2022, 43, 2148-2163.	3.6	5
47	A new PET detector concept for compact preclinical high-resolution hybrid MR-PET. Nuclear Instruments and Methods in Physics Research, Section A: Accelerators, Spectrometers, Detectors and Associated Equipment, 2018, 888, 44-52.	1.6	4
48	Image-based Motion Correction for the Siemens hybrid-MR/BrainPET Scanner. Nuklearmedizin - NuclearMedicine, 2019, 58, .	0.7	4
49	The Gamma Functional Navigator. IEEE Transactions on Nuclear Science, 2004, 51, 682-689.	2.0	3
50	Front-end circuit for position sensitive silicon and vacuum tube photomultipliers with gain control and depth of interaction measurement. Nuclear Instruments and Methods in Physics Research, Section A: Accelerators, Spectrometers, Detectors and Associated Equipment, 2007, 576, 118-122.	1.6	3
51	AMIC: An expandable front-end for gamma-ray detectors with light distribution analysis capabilities. , 2010, , .		3
52	Sensitivity Encoded Silicon Photomultipliers (SeSPs): A novel detector design for uniform crystal identification. , 2011, , .		3
53	NIMG-32. DIFFERENTIATION OF PSEUDOPROGRESSION FROM TUMOR PROGRESSION IN GLIOBLASTOMA PATIENTS BASED ON FET PET RADIOMICS. Neuro-Oncology, 2017, 19, vi148-vi149.	1.2	3
54	Corrected position estimation in PET detector modules with multi-anode PMTs using neural networks. , 2005, , .		2

CHRISTOPH LERCHE

#	Article	IF	CITATIONS
55	Singles and coincidence processing for a digital PET/MR system using SiPM detectors. , 2011, , .		2
56	MR image quality and timing resolution of an analog SiPM based pre-clinical PET/MR insert. , 2012, , .		2
57	A Linearized Fit Model for Robust Shape Parameterization of FET-PET TACs. IEEE Transactions on Medical Imaging, 2021, 40, 1-1.	8.9	2
58	Efficient readout electronics for multi-anode photomultiplier. , 2010, , .		1
59	PET performance evaluation of a pre-clinical SiPM based MR-compatible PET scanner. , 2012, , .		1
60	Demonstration of motion correction for PET-MR with PVA cryogel phantoms. , 2013, , .		1
61	New Imaging Method of Positrons Leaving the Source Application for PET/MR hybrid Scanners , 2017, ,		1
62	NIMG-82. PREDICTING ISOCITRATE DEHYDROGENASE GENOTYPE IN GLIOMAS USING FET PET RADIOMICS. Neuro-Oncology, 2017, 19, vi160-vi160.	1.2	1
63	Variable preprocessing applied to neural network position estimators for 2-D PET. , 2011, , .		0
64	Reconstruction of attenuation maps for a PET/MR scanner based on the LSO background activity. , 2015, , .		0
65	Attenuation Correction of Cerebellum in PET/MR Data. , 2017, , .		Ο
66	Iterative, direct LOR PET Image Reconstruction of Human Brain Data for the Siemens mMR Biograph. , 2017, , .		0
67	Full dynamic brain simulation using GATE in a high-performance computer. , 2017, , .		Ο
68	Resolution Modelling in Projection Space using Factorized Multi-block Detector Response Function. , 2018, , .		0
69	RESampling between Projection SpACEs (RESPACE) using Bayse' Theorem. , 2018, , .		0
70	Event reconstruction in NEW using a ML-EM algorithm. , 2017, , .		0
71	A software-based approach for calculating spatially resolved radiation exposure for structural radiation protection in nuclear medical imaging. Journal of Radiological Protection, 0, , .	1.1	0