
German Augusto GÃ³mez-RÃ-os

List of Publications by Year in descending order

Source: https://exaly.com/author-pdf/8605569/publications.pdf

Version: 2024-02-01

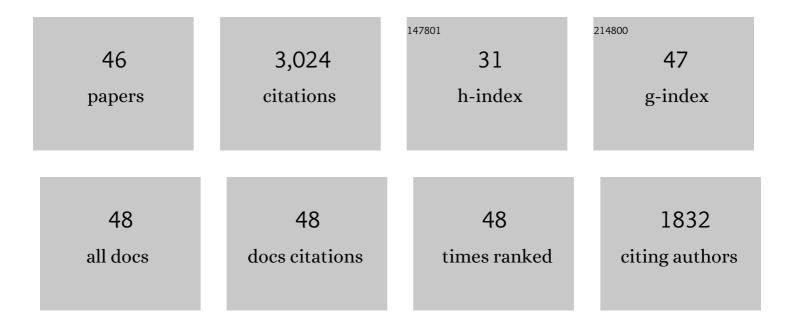

#	Article	IF	CITATIONS
1	Advances in Solid Phase Microextraction and Perspective on Future Directions. Analytical Chemistry, 2018, 90, 302-360.	6.5	534
2	A critical review of the state of the art of solid-phase microextraction of complex matrices III. Bioanalytical and clinical applications. TrAC - Trends in Analytical Chemistry, 2015, 71, 249-264.	11.4	203
3	Development of Coated Blade Spray Ionization Mass Spectrometry for the Quantitation of Target Analytes Present in Complex Matrices. Angewandte Chemie - International Edition, 2014, 53, 14503-14507.	13.8	201
4	SPME – Quo vadis?. Analytica Chimica Acta, 2012, 750, 132-151.	5.4	163
5	Biocompatible Solid-Phase Microextraction Nanoelectrospray Ionization: An Unexploited Tool in Bioanalysis. Analytical Chemistry, 2016, 88, 1259-1265.	6.5	117
6	Solid phase microextraction (SPME)-transmission mode (TM) pushes down detection limits in direct analysis in real time (DART). Chemical Communications, 2014, 50, 12937-12940.	4.1	113
7	Ultrafast Screening and Quantitation of Pesticides in Food and Environmental Matrices by Solid-Phase Microextraction–Transmission Mode (SPME-TM) and Direct Analysis in Real Time (DART). Analytical Chemistry, 2017, 89, 7240-7248.	6.5	111
8	Fast Quantitation of Target Analytes in Small Volumes of Complex Samples by Matrix ompatible Solidâ€Phase Microextraction Devices. Angewandte Chemie - International Edition, 2016, 55, 7510-7514.	13.8	96
9	Open Port Probe Sampling Interface for the Direct Coupling of Biocompatible Solid-Phase Microextraction to Atmospheric Pressure Ionization Mass Spectrometry. Analytical Chemistry, 2017, 89, 3805-3809.	6.5	88
10	Solid Phase Microextraction-mass spectrometry: Metanoia. TrAC - Trends in Analytical Chemistry, 2019, 112, 201-211.	11.4	76
11	High-Throughput Screening and Quantitation of Target Compounds in Biofluids by Coated Blade Spray-Mass Spectrometry. Analytical Chemistry, 2017, 89, 8421-8428.	6.5	73
12	Quantitative analysis of biofluid spots by coated blade spray mass spectrometry, a new approach to rapid screening. Scientific Reports, 2017, 7, 16104.	3.3	73
13	Towards on-site analysis of complex matrices by solid-phase microextraction-transmission mode coupled to a portable mass spectrometer via direct analysis in real time. Analyst, The, 2017, 142, 2928-2935.	3.5	67
14	Single-Use Poly(etheretherketone) Solid-Phase Microextraction–Transmission Mode Devices for Rapid Screening and Quantitation of Drugs of Abuse in Oral Fluid and Urine via Direct Analysis in Real-Time Tandem Mass Spectrometry. Analytical Chemistry, 2018, 90, 952-960.	6.5	58
15	Hunting Molecules in Complex Matrices with SPME Arrows: A Review. Separations, 2020, 7, 12.	2.4	56
16	Development of a Microfluidic Open Interface with Flow Isolated Desorption Volume for the Direct Coupling of SPME Devices to Mass Spectrometry. Analytical Chemistry, 2018, 90, 2631-2638.	6.5	50
17	Rapid determination of immunosuppressive drug concentrations in whole blood by coated blade spray-tandem mass spectrometry (CBS-MS/MS). Analytica Chimica Acta, 2018, 999, 69-75.	5.4	49
18	Low invasive in vivo tissue sampling for monitoring biomarkers and drugs during surgery. Laboratory Investigation, 2014, 94, 586-594.	3.7	47

#	Article	IF	CITATIONS
19	In Vivo Brain Sampling Using a Microextraction Probe Reveals Metabolic Changes in Rodents after Deep Brain Stimulation. Analytical Chemistry, 2019, 91, 9875-9884.	6.5	47
20	Solid phase microextraction fills the gap in tissue sampling protocols. Analytica Chimica Acta, 2013, 803, 75-81.	5.4	46
21	Fast quantitation of opioid isomers in human plasma by differential mobility spectrometry/mass spectrometry via SPME/open-port probe sampling interface. Analytica Chimica Acta, 2017, 991, 89-94.	5.4	46
22	Breaching the 10 Second Barrier of Total Analysis Time for Complex Matrices via Automated Coated Blade Spray. Analytical Chemistry, 2019, 91, 13039-13046.	6.5	43
23	Coated blade spray: shifting the paradigm of direct sample introduction to MS. Bioanalysis, 2018, 10, 257-271.	1.5	41
24	Deposition of a Sorbent into a Recession on a Solid Support To Provide a New, Mechanically Robust Solid-Phase Microextraction Device. Analytical Chemistry, 2017, 89, 8021-8026.	6.5	40
25	Optimization of Coated Blade Spray for Rapid Screening and Quantitation of 105 Veterinary Drugs in Biological Tissue Samples. Analytical Chemistry, 2020, 92, 5937-5943.	6.5	40
26	Ultra-fast quantitation of voriconazole in human plasma by coated blade spray mass spectrometry. Journal of Pharmaceutical and Biomedical Analysis, 2017, 144, 106-111.	2.8	37
27	Direct coupling of solid phase microextraction with electrospray ionization mass spectrometry: A Case study for detection of ketamine in urine. Analytica Chimica Acta, 2019, 1075, 112-119.	5.4	37
28	Coupling needle trap devices with gas chromatography–ion mobility spectrometry detection as a simple approach for on-site quantitative analysis. Journal of Chromatography A, 2013, 1300, 193-198.	3.7	35
29	Development of Needle Trap Technology for On-Site Determinations: Active and Passive Sampling. Analytical Chemistry, 2014, 86, 5889-5897.	6.5	35
30	Solid Phase Microextraction On-Fiber Derivatization Using a Stable, Portable, and Reusable Pentafluorophenyl Hydrazine Standard Gas Generating Vial. Analytical Chemistry, 2016, 88, 6859-6866.	6.5	33
31	Rapid determination of tacrolimus and sirolimus in whole human blood by direct coupling of solid-phase microextraction to mass spectrometry via microfluidic open interface. Analytica Chimica Acta, 2021, 1144, 53-60.	5.4	33
32	Rapid and Concomitant Analysis of Pharmaceuticals in Treated Wastewater by Coated Blade Spray Mass Spectrometry. Environmental Science & Technology, 2017, 51, 12566-12572.	10.0	31
33	High-throughput analysis using non-depletive SPME: challenges and applications to the determination of free and total concentrations in small sample volumes. Scientific Reports, 2018, 8, 1167.	3.3	31
34	Solid phase microextraction coupled to mass spectrometry <i>via</i> a microfluidic open interface for rapid therapeutic drug monitoring. Analyst, The, 2019, 144, 3721-3728.	3.5	28
35	Evaluation of a coated blade spray-tandem mass spectrometry assay as a new tool for the determination of immunosuppressive drugs in whole blood. Analytical and Bioanalytical Chemistry, 2020, 412, 5067-5076.	3.7	24
36	Comprehensive Investigation of Metabolic Changes Occurring in the Rat Brain Hippocampus after Fluoxetine Administration Using Two Complementary In Vivo Techniques: Solid Phase Microextraction and Microdialysis. ACS Chemical Neuroscience, 2020, 11, 3749-3760.	3.5	24

#	Article	IF	CITATIONS
37	Highâ€throughput quantification of drugs of abuse in biofluids via 96â€solidâ€phase microextraction–transmission mode and direct analysis in real time mass spectrometry. Rapid Communications in Mass Spectrometry, 2019, 33, 1423-1433.	1.5	23
38	Space-Resolved Tissue Analysis by Solid-Phase Microextraction Coupled to High-Resolution Mass Spectrometry via Desorption Electrospray Ionization. Analytical Chemistry, 2019, 91, 10141-10148.	6.5	22
39	Analysis of endocannabinoids in plasma samples by biocompatible solid-phase microextraction devices coupled to mass spectrometry. Analytica Chimica Acta, 2019, 1091, 135-145.	5.4	22
40	Investigation of Early Death-Induced Changes in Rat Brain by Solid Phase Microextraction via Untargeted High Resolution Mass Spectrometry: <i>In Vivo</i> versus Postmortem Comparative Study. ACS Chemical Neuroscience, 2020, 11, 1827-1840.	3.5	19
41	Assessment of solid phase microextraction as a sample preparation tool for untargeted analysis of brain tissue using liquid chromatography-mass spectrometry. Journal of Chromatography A, 2021, 1638, 461862.	3.7	18
42	Evaluation of a multiâ€fiber exchange solidâ€phase microextraction system and its application to onâ€site sampling. Journal of Separation Science, 2015, 38, 3560-3567.	2.5	17
43	Development of a standard gas generating vial comprised of a silicon oil–polystyrene/divinylbenzene composite sorbent. Journal of Chromatography A, 2015, 1410, 1-8.	3.7	17
44	Development of a new inâ€vial standard gas system for calibrating solidâ€phase microextraction in highâ€throughput and onâ€site applications. Journal of Separation Science, 2013, 36, 2939-2945.	2.5	15
45	Fast Quantitation of Target Analytes in Small Volumes of Complex Samples by Matrix ompatible Solidâ€Phase Microextraction Devices. Angewandte Chemie, 2016, 128, 7636-7640.	2.0	11
46	Analysis of food samples made easy by microextraction technologies directly coupled to mass spectrometry. Journal of Mass Spectrometry, 2021, 56, e4665.	1.6	7